



## ATLAS Malaria *Plasmodium falciparum* Rapid Test Device (Whole Blood)

A rapid test for the qualitative detection of circulating *plasmodium falciparum* (P.f.) in whole blood.

For professional *in vitro* diagnostic use only.

### INTENDED USE

Atlas Malaria P.f. Rapid Test Device (Whole Blood) is a rapid chromatographic immunoassay for the qualitative detection of circulating *plasmodium falciparum* in whole blood.

### SUMMARY

Malaria is caused by a protozoan which invades human red blood cells.<sup>1</sup> Malaria is one of the world's most prevalent diseases. According to the WHO, the worldwide prevalence of the disease is estimated to be 300-500 million cases and over 1 million deaths each year. Most of these victims are infants and young children. Over half of the world's population lives in malarious areas. Microscopic analysis of appropriately stained thick and thin blood smears has been the standard diagnostic technique for identifying malaria infections for more than a century.<sup>2</sup> The technique is capable of accurate and reliable diagnosis when performed by skilled microscopists using defined protocols. The skill of the microscopist and use of proven and defined procedures, frequently present the greatest obstacles to fully achieving the potential accuracy of microscopic diagnosis. Although there is a logistical burden associated with performing a time-intensive, labor-intensive, and equipment-intensive procedure such as diagnostic microscopy, it is the training required to establish and sustain competent performance of microscopy that poses the greatest difficulty in employing this diagnostic technology.

Atlas Malaria P.f. Rapid Test Device (Whole Blood) is a rapid test to qualitatively detect the presence of the P.f. antigen. The test utilizes gold conjugate to selectively detect P.f. antigen in whole blood.

### PRINCIPLE

Atlas Malaria P.f. Rapid Test Device (Whole Blood) is a

qualitative, membrane based immunoassay for the detection of P.f. antigen in whole blood. The membrane is pre-coated with P.f. antibody. During testing, the whole blood specimen reacts with the dye conjugate, which has been pre-coated in the test strip. The mixture then migrates upward on the membrane chromatographically by capillary action and reacts with P.f. antibody on the membrane on the test line. If the specimen contains P.f. antigen, a red line will appear in the test region. The absence of the red line in test region indicates that the specimen does not contain P.f. antigen. To serve as a procedural control, a red line will always appear in the control region indicating that proper volume of specimen has been added and membrane wicking has occurred.

### REAGENTS

The test device contains monoclonal Malaria antibody coated on the membrane.

### PRECAUTIONS

- For professional *in vitro* diagnostic use only. Do not use after expiration date.
- For whole blood specimen use only. Do not use other specimens.
- Do not eat, drink or smoke in the area where the specimens or kits are handled.
- Handle all specimens as if they contain infectious agents. Observe established precautions against microbiological hazards throughout all procedures and follow the standard procedures for proper disposal of specimens.
- Wear protective clothing such as laboratory coats, disposable gloves and eye protection when specimens are assayed.
- Humidity and temperature can adversely affect results.

### STORAGE AND STABILITY

The kit can be stored at room temperature or refrigerated (2-30°C). The test device is stable through the expiration date printed on the sealed pouch. The test device must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use beyond the expiration date.

### SPECIMEN COLLECTION AND PREPARATION

- Atlas Malaria P.f. Rapid Test Device (Whole Blood) can be performed using whole blood.
- Both Fingerstick Whole Blood and Venipuncture Whole Blood can be used.
- To collect Fingerstick Whole Blood specimens:
  - Wash the patient's hand with soap and warm water or clean with an

alcohol swab. Allow to dry.

- Massage the hand without touching the puncture site by rubbing down the hand towards the fingertip of the middle or ring finger.
  - Puncture the skin with a sterile lancet. Wipe away the first sign of blood.
  - Gently rub the hand from wrist to palm to finger to form a rounded drop of blood over the puncture site.
- Testing should be performed immediately after specimen collection. Do not leave the specimens at room temperature for prolonged periods. Whole blood collected by venipuncture should be stored at 2-8°C if the test is to be run within 2 days of collection. Do not freeze whole blood specimens. Whole blood collected by fingerstick should be tested immediately.
  - Bring specimens to room temperature prior to testing.
  - If specimens are to be shipped, they should be packed in compliance with federal regulations covering the transportation of etiologic agents.

### MATERIALS

#### Materials Provided

- Test devices
- Disposable specimen droppers
- Buffer
- Package insert

#### Materials Required But Not Provided

- Pipette and disposable tips (optional)
- Specimen collection containers
- Lancets (for fingerstick whole blood only)
- Timer


### DIRECTIONS FOR USE

**Allow the test device, specimen, buffer, and/or controls to equilibrate to room temperature (15-30°C) prior to testing.**

1. Remove the test device from the foil pouch and use it as soon as possible. Best results will be obtained if the assay is performed within one hour.
2. Place the test device on a clean and level surface. Transfer the specimen by a pipette or a dropper:
  - To use a **Pipette**: Transfer 10 µL of whole blood to the specimen well (S) of the test device, then add 3 full drops of buffer (approximately 120 µL) and start the timer. Avoid trapping air bubbles in the specimen well (S). See illustration □ below.
  - To use a **Disposable Specimen Dropper**: Hold the

dropper vertically, draw the specimen up to the Fill Line as shown in illustration □ below (approximately 10 µL). Transfer the specimen to the specimen well (S) of the test device, then add 3 full drops of buffer (approximately 120 µL) and start the timer. Avoid trapping air bubbles in the specimen well (S).

- Wait for the red line(s) to appear. The result should be read at 15 minutes. Do not interpret the result after 20 minutes.

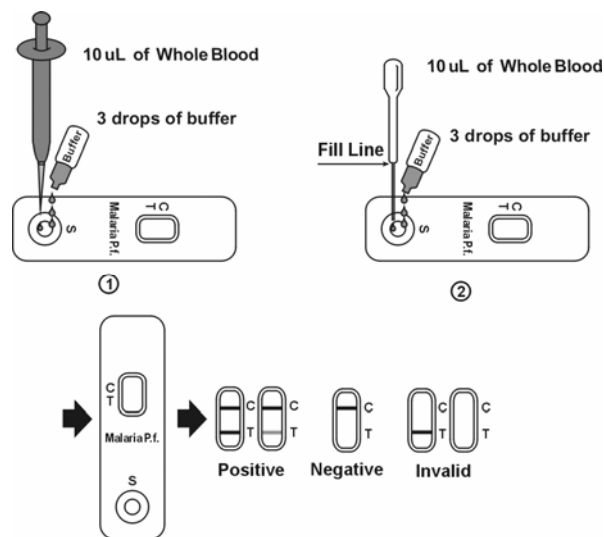

## INTERPRETATION OF RESULTS

(Please refer to the illustration above)

**POSITIVE:** \* **Two distinct red lines appear.** One line should be in the control region (C) and another line should be in the test region (T).

**\*NOTE:** The intensity of the red color in the test line region (T) may vary depending on the concentration of P.f. present in the specimen. Therefore, any shade of red in the test region (T) should be considered positive.

**NEGATIVE:** **One red line appears in the control region (C).** No apparent red or pink line appears in the test region (T).

**INVALID:** **Control line fails to appear.** Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test device. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

## QUALITY CONTROL

Internal procedural controls are included in the test. A red line appearing in the control region (C) is an internal positive procedural control. It confirms sufficient specimen volume and correct procedural technique.

Control standards are not supplied with this kit; however, it is recommended that positive and negative controls be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

## LIMITATIONS

- Atlas Malaria P.f. Rapid Test Device (Whole Blood) is for *in vitro* diagnostic use only. This test should be used for the detection of P.f. antigen in whole blood specimens only. Neither the quantitative value nor the rate of increase in P.f. antigen concentration can be determined by this qualitative test.
- Atlas Malaria P.f. Rapid Test Device (Whole Blood) will only indicate the presence of P.f. antigen in the specimen and should not be used as the sole criteria for the diagnosis of malaria infection.
- As with all diagnostic tests, all results must be interpreted together with other clinical information available to the physician.
- If the test result is negative and clinical symptoms persist, additional testing using other clinical methods is recommended. A negative result does not at any time preclude the possibility of malarial infection.

## PERFORMANCE CHARACTERISTICS

### Sensitivity

Atlas Malaria P.f. Rapid Test Device (Whole Blood) has been tested with thin and thick blood smears on clinical samples. The results show that the sensitivity of Atlas Malaria P.f. Rapid Test Device (Whole Blood) is over 99.0% relative to blood smears.

### Specificity

Atlas Malaria P.f. Rapid Test Device (Whole Blood) uses an antibody that is highly specific for Malaria P.f. antigen in whole blood. The results show that the specificity of Atlas Malaria P.f. Rapid Test Device (Whole Blood) is over 99.0% relative to blood smears.

Method	Blood Smears		Total Results
	Positive	Negative	
Malaria P.f. Rapid Test Device	Positive	93	93
	Negative	0	239

Total Results	93	239	332
---------------	----	-----	-----

Relative Sensitivity: >99.0%

Relative Specificity: >99.0%

Accuracy: >99.0%

## Precision

### Intra Assay

The run precision has been determined by using 15 replicates of three specimens containing negative, low positive and high positive samples. The negative and positive values were correctly identified 99.8% of the time.

### Inter Assay

Between run precision has been determined by using the same three specimens of negative, low positive and high positive of 15 independent assays and with three different lots of Atlas Malaria P.f. Rapid Test Device (Whole Blood) over a 3 month period. The negative and positive values were correctly identified 99.8% of the time.

## BIBLIOGRAPHY

- Bill McConell, *Malaria Laboratory Diagnosis*. January 2001
- Cooke AH, Chiodini PL, Doherty T, et al, *Comparison of a parasite lactate dehydrogenase-base immunochromatographic antigen detection assay with microscopy for the detection of malaria parasite in human blood samples*. Am J Trop Med Hyp, 1999, Feb: 60(2):173-2

ATLAS MEDICAL

Unit 4, William James House

Cowley Rd, Cambridge, CB4 0WX

**Tel: ++44 (0) 1223 858 910**

**Fax: ++44 (0) 1223 858 524**

PPI100A01

Revision B (15.08.2004)