



Carcinoembryonic Antigen (CEA) Enzyme Immunoassay Kit

Enzyme Immunoassay for the Quantitative Determination of Carcinoembryonic Antigen (CEA) in Human Serum

For *In-Vitro* and professional use
Store at 2 to 8°C.

PROPRIETARY AND COMMON NAMES

CEA Enzyme Immunoassay

INTENDED USE

For the quantitative determination of the Cancer Antigen CEA concentration in human serum.

INTRODUCTION

Carcinoembryonic antigen (CEA) is a cell-surface 200-kd glycoprotein. In 1969, it was reported that plasma CEA was elevated in 35 of 36 patients with adenocarcinoma of the colon and that CEA titers decreased after successful surgery. Normal levels were observed in all patients with other forms of cancer or benign diseases. Subsequent studies have not confirmed these initial findings, and it is now understood that elevated levels of CEA are found in many cancers. Increased levels of CEA are observed in more than 30% of patients with cancer of the lung, liver, pancreas, breast, colon, head or neck, bladder, cervix, and prostate. Elevated plasma levels are related to the stage and extent of the disease, the degree of differentiation of the tumor, and the site of metastasis. CEA is also found in normal tissue.

PRINCIPLE OF THE TEST

The CEA ELISA test is based on the principle of a solid phase enzyme-linked immunosorbent assay. The assay system utilizes a monoclonal antibody directed against a distinct antigenic determinant on the intact CEA molecule is used for solid phase immobilization (on the microtiter wells). A goat anti-CEA antibody conjugated to horseradish peroxidase (HRP) is in the antibody-enzyme conjugate solution. The test sample is allowed to react simultaneously with the two antibodies, resulting in the CEA molecules being sandwiched between the solid phase and enzyme-linked antibodies. After a 1 hour incubation at room temperature, the wells are washed with water to remove unbound labeled antibodies. A solution of TMB Reagent is added and incubated for 20 minutes, resulting in the development of a blue color. The color development is stopped with the addition of Stop Solution changing the color to yellow. The concentration of

CEA is directly proportional to the color intensity of the test sample. Absorbance is measured spectrophotometrically at 450nm.

REAGENTS

Materials provided with the kit:

- Antibody-coated microtiter plate with 96 wells.
- Lyophilized CEA standards containing; 0, 3, 12, 30, 60, and 120 ng/ml CEA. 1 set.
- Enzyme Conjugate Reagent, 13 ml.
- TMB Reagent (One-Step), 11 ml.
- Stop Solution (1 N HCl), 11 ml.

Materials required but not provided:

- Precision pipettes: 50 µl, 100 µl, and 1 µl.
- Disposable pipette tips.
- Distilled water.
- Vortex mixer or equivalent.
- Absorbent paper or paper towel.
- Graph paper.
- Microtiter plate reader.

SPECIMEN COLLECTION AND PREPARATION

Serum should be prepared from a whole blood specimen obtained by acceptable medical techniques. This kit is for use with serum samples without additives only.

STORAGE OF TEST KIT AND INSTRUMENTATION

Unopened test kits should be stored at 2-8°C upon receipt and the microtiter plate should be kept in a sealed bag with desiccants to minimize exposure to damp air. Opened test kits will remain stable until the expiration date shown, provided it is stored as described above. A microtiter plate reader with a bandwidth of 10 nm or less and an optical density range of 0-2 OD or greater at 450 nm wavelength is acceptable for use in absorbance measurement.

REAGENT PREPARATION

1. All reagents should be brought to room temperature (18-25°C) before use.
2. Reconstitute each lyophilized standard with 1.0 ml distilled water. Allow the reconstituted material to stand for at least 20 minutes and mix gently. Reconstituted standards will be stable for up to 30 days when stored sealed at 2-8°C.
3. **Hook Effect:** *In order to avoid hook effect, samples with expected CEA concentrations over 9,000 ng/ml may be quantitated by 100-fold (i.e. 0.01 ml to 1.0 ml) dilution with CEA-free human serum.*

ASSAY PROCEDURE

1. Secure the desired number of coated wells in the holder.
2. Dispense 50 µl of standard, specimens, and controls into appropriate wells.
3. Dispense 100 µl of Enzyme Conjugate Reagent to each well.
4. Thoroughly mix for 30 seconds. It is very important to have a complete mixing in this setup.

5. Incubate at room temperature (18-25°C) for 60 minutes.
6. Remove the incubation mixture by emptying plate content into a waste container.
7. Rinse and empty the microtiter wells 5 times with distilled or deionized water. (Please do not use tap water.)
8. Strike the wells sharply onto absorbent paper or paper towels to remove all residual water droplets.
9. Dispense 100 µl of TMB Reagent into each well. Gently mix for 10 seconds.
10. Incubate at room temperature for 20 minutes.
11. Stop the reaction by adding 100 µl of Stop Solution to each well.
12. Gently mix for 30 seconds. ***It is important to make sure that all the blue color changes to yellow color completely.***
13. Read the optical density at 450 nm with a microtiter plate reader within 15 minutes.


CALCULATION OF RESULTS

1. Calculate the average absorbance values (A₄₅₀) for each set of reference standards, control, and samples.
2. Construct a standard curve by plotting the mean absorbance obtained for each reference standard against its concentration in ng/ml on linear graph paper, with absorbance on the vertical (y) axis and concentration on the horizontal (x) axis.
3. Using the mean absorbance value for each sample, determine the corresponding concentration of CEA in ng/ml from the standard curve.
4. ***Any values obtained for diluted samples must be further converted by applying the appropriate dilution factor in the calculation.***

EXAMPLE OF STANDARD CURVE

Results of a typical standard run with optical density readings at 450 nm shown in the Y axis against CEA concentrations shown in the X axis. This standard curve is for the purpose of illustration only, and should not be used to calculate unknowns. Each user should obtain his or her own data and standard curve.

CEA (ng/ml)	Absorbance (450 nm)
0	0.067
3	0.191
12	0.578
30	1.040
60	1.797
120	2.647

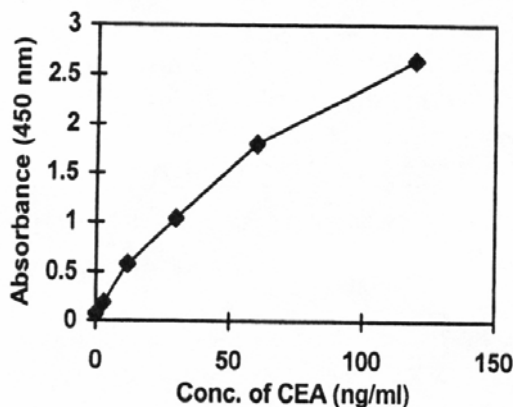

EXPECTED VALUES AND SENSITIVITY

The most complete study of CEA is a compilation of collaborative studies in which CEA values in 35,000 samples from more than 10,000 patients and controls were analyzed. Of 1425 normal persons who did not smoke, 98.7% had values less than 5.0 ng/ml. It is recommended that each laboratory establish its own normal range.

The minimum detectable concentration of CEA by this assay is estimated to be 1.0 ng/ml.

LIMITATIONS OF THE PROCEDURE

1. Reliable and reproducible results will be obtained when the assay procedure is carried out with a complete understanding of the package insert instructions and with adherence to good laboratory practice.
2. The wash procedure is critical. Insufficient washing will result in poor precision and falsely elevated absorbance readings.
3. Serum samples demonstrating gross lipemia, gross hemolysis, or turbidity should not be used with this test.
4. The results obtained from the use of this kit should be used only as an adjunct to other diagnostic procedures and information available to the physician.

REFERENCES

- 1 Engall, E., Methods in Enzymology, Volume 70, Van Vunakis, H. and Langone, J. J. (eds.), Academic Press, New York, 419-492(1980).
- 2 Uotila, M., Ruoslahti, E. and Engvall, E., J. Immunol. Methods, 42, 11-15 (1981).
- 3 Gold P, Freedman S O. Demonstration of tumor specific antigen in human colonic carcinoma by immunologic tolerance and absorption techniques. J Exp Med 1965;127:439-462.
- 4 Thompson D P M, Krupey J, Freedman S O, et al. The radioimmunoassay of circulating carcinoembryonic antigen of the human digestive system. Proc Natl Acad Sci USA 1969;64:161-167.
- 5 Schwartz M K. Tumor markers in diagnosis and screening. In: Ting S W, Chen J S, Schwartz M K, eds. Human tumor markers, Amsterdam: Elsevier Science, 1987;3-16.
- 6 Zamcheck N. and Martin E.W. Sequential Carcinoembryonic Antigen Levels in Pancreatic Cancer: Some Clinical Correlations. Cancer 1981;47:1620-1627.
- 7 Mughal A.W., Hortobagyi G. N., Fritsche H.A., Buzdar A.U. Yap H-Y., and Blumenschein G.R. Serial Plasma Carcinoembryonic Antigen Measurements During Treatment of Metastatic Breast Cancer. JAMA 1983; 259:1881-1886.

ATLAS Medical
William James House,
Cowley Road, Cambridge, CB4 4WX, UK
 Tel: ++44 (0) 1223 858 910
 Fax: ++44 (0) 1223 858 524

PPI198A01
Revision A (26.06.2005)